


# X-Cell – Electrochemical test cell

## Overview & assembly manual

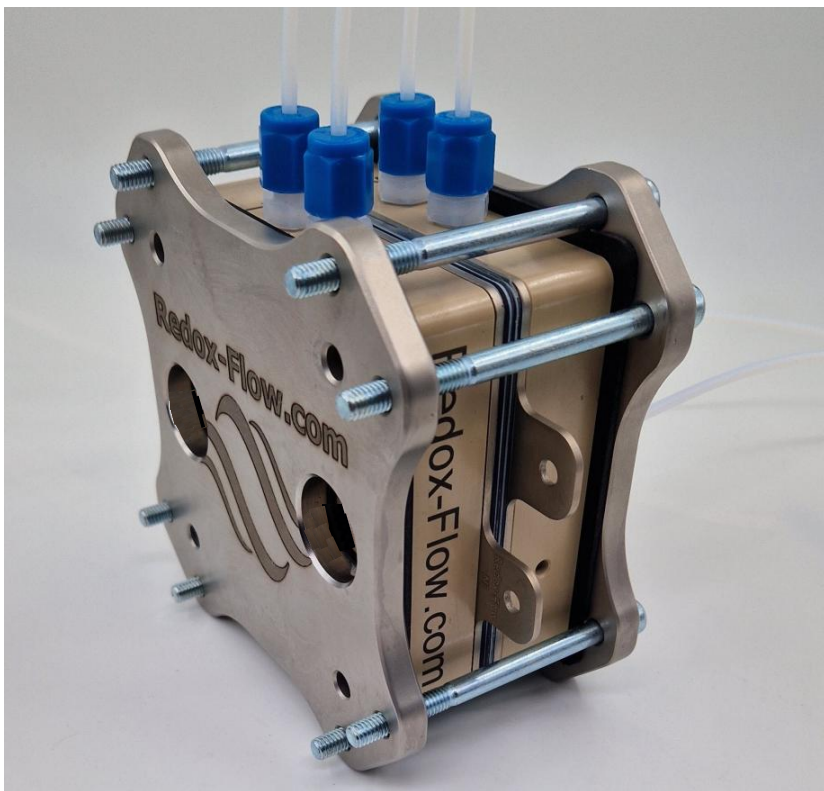

Version date	March 27 – 2025
Manual version	4.0 - visit <a href="http://www.redox-flow.com">www.redox-flow.com</a> for updated versions and spare parts
Notes	This equipment is intended for research purposes only and can be applied for different purposes. There is no guarantee on performance, corrosion or lifetime of the equipment. See <a href="https://redox-flow.com/termsandconditions/">https://redox-flow.com/termsandconditions/</a> for more information.

# Overview of variants & components included in the cell package

## General notes

- All gaskets are ordered separately – are available in PTFE, EPDM and VITON  
NOTE: Gaskets are here generally depicted as white (PTFE), however, VITON and EPDM are black.
- Cells are delivered with ring-gaskets and o-rings in both EPDM and VITON
- Current collectors comes in standard materials (see [www.redox-flow.com](http://www.redox-flow.com) for materials).
- Membranes and electrodes are not included in the cell package – can be ordered separately



Flat bottom flangeless fittings and blinds (1/4-28 UNF)



Ring gaskets (in EPDM and VITON)




PEEK alignment bars




Bolts

## Current collectors with flat surface

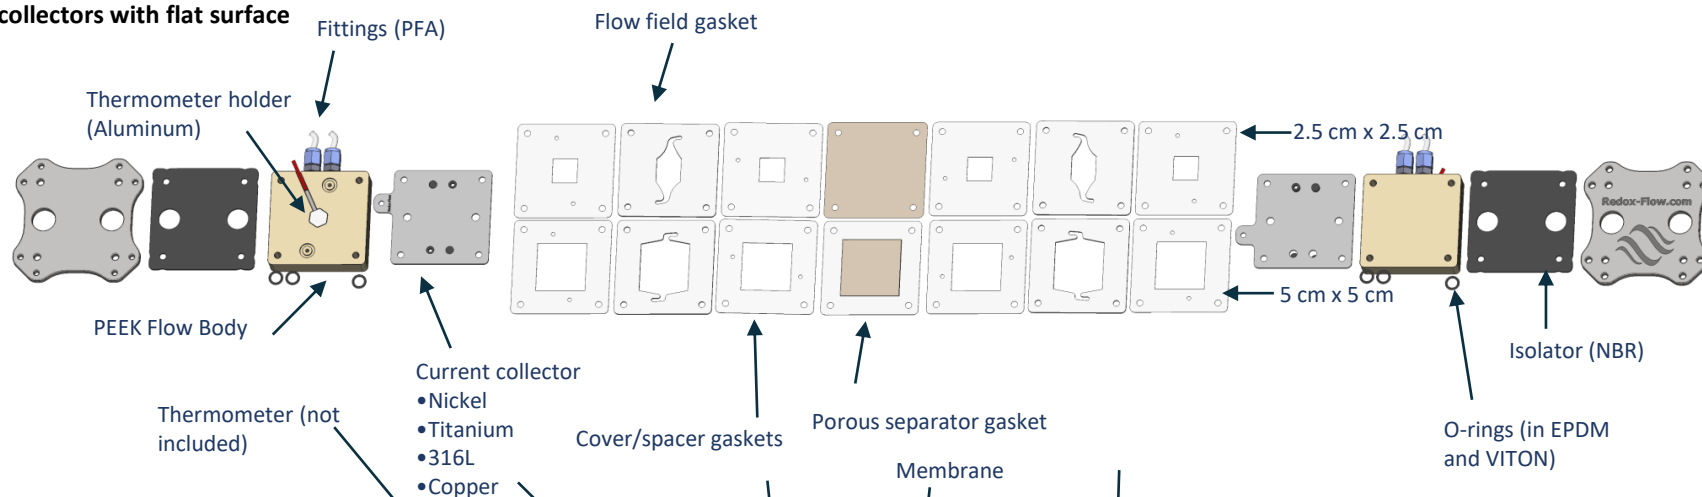

## Current collectors with flow field

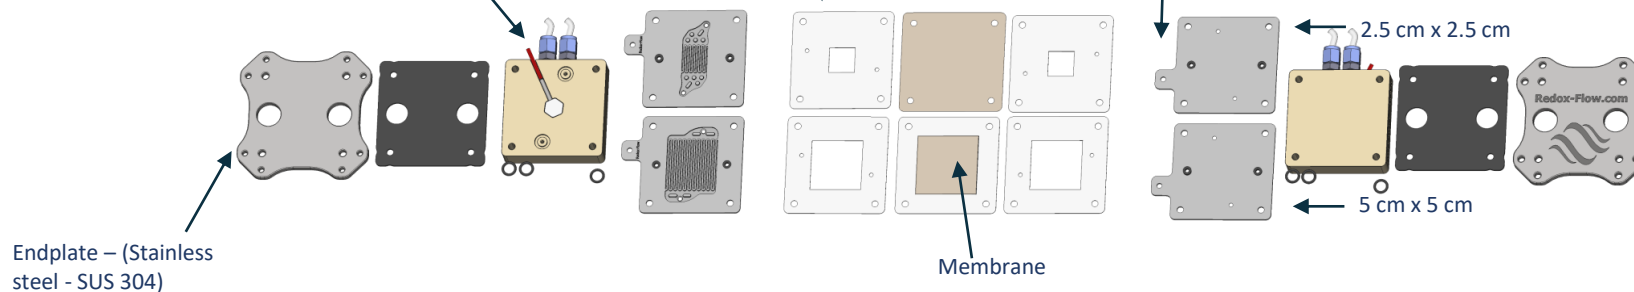


# Assembly


- Image below shows the overall assembly of the cell for both 2.5cm x 2.5cm and 5cm x 5cm active area.
- Assembly goes from left to right with the components turned and rotated as shown in the image.
- Following pages shows a detailed description

NOTE: The order of assembly does not strictly need to follow this manual. Depending on use and experience, assembly can deviate from this manual.



## Current collectors with flat surface

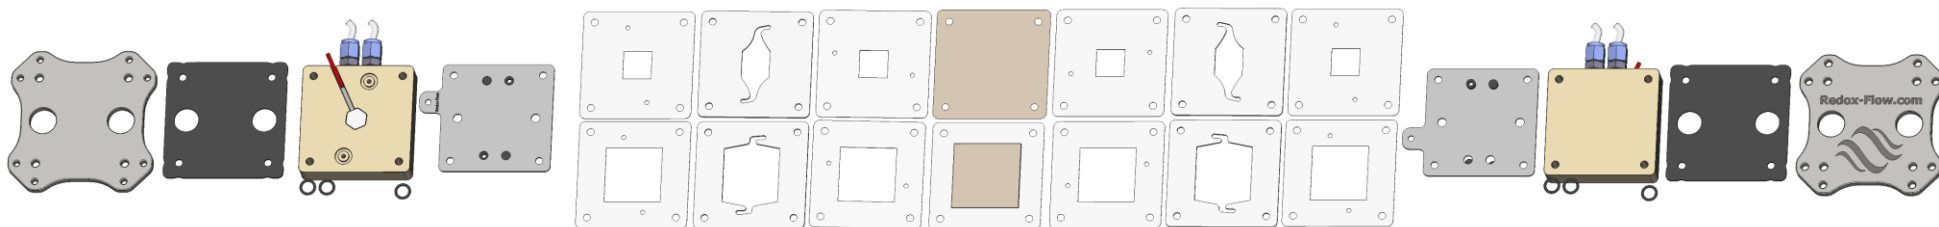

## Current collectors with flow field

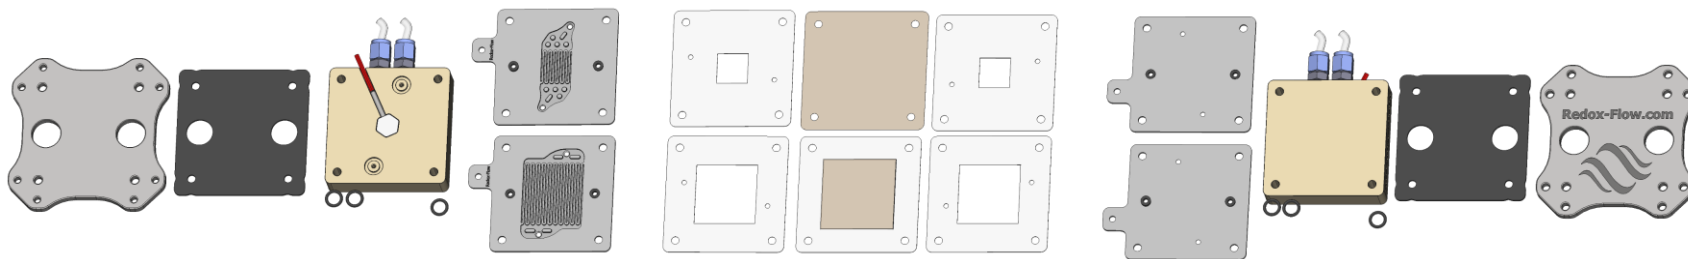


# Assembly - Current collectors with flat surface

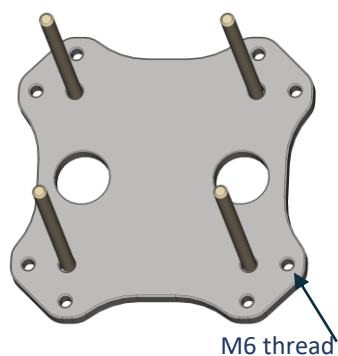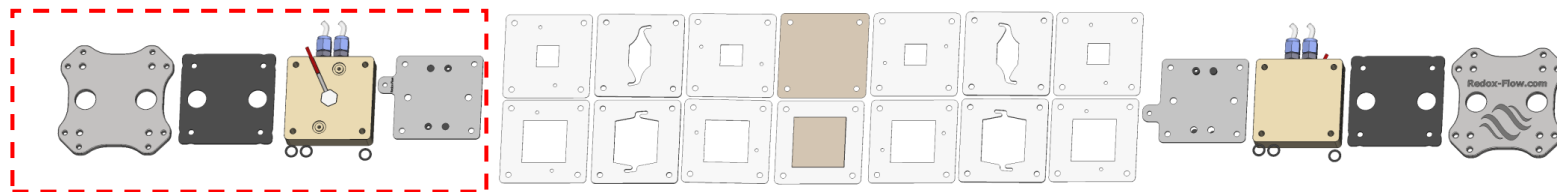


1. Threaded endplate is placed with logo downwards

2. All four alignment bars are placed in the holes in the endplate

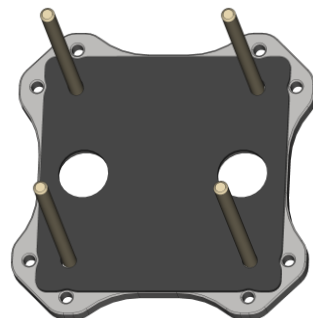


3. Isolator is placed on endplate

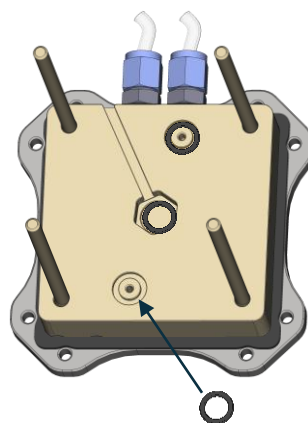


4. PEEK flow body is placed on isolator

5. All three O-rings are mounted in the PEEK flow body

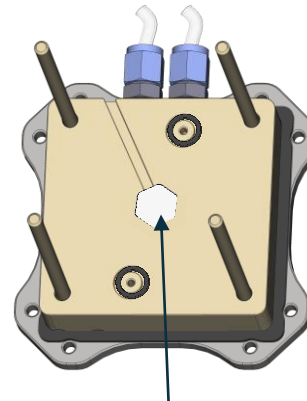

6. Alu thermometer holder is placed in the center hole


NOTE: The holder comes with three holes with different diameter.  
-Choose the hole that fits your thermometer best  
-Make sure the hole points toward the groove in the PEEK plate  
-To ensure good thermal contact a little grease can be applied in the hole.

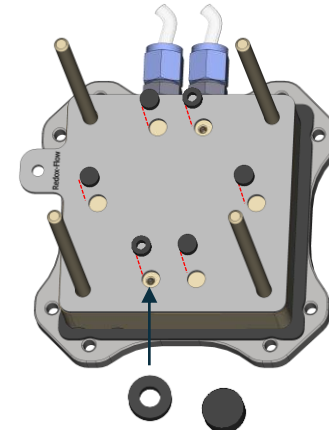



7. Current collector is placed on PEEK flow body

8. *Ring gaskets* with and without holes are mounted in current collector. Use


NOTE: Use *Ring gaskets* with holes where there is a port and *Ring gaskets* without holes in the holes without ports.

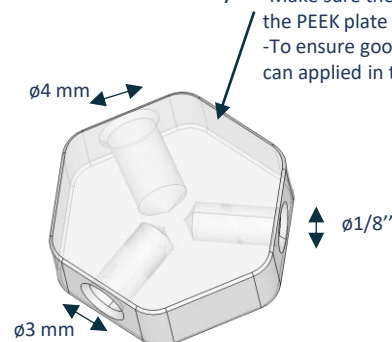


# Assembly - Current collectors with flat surface

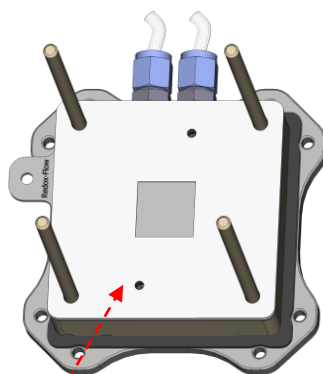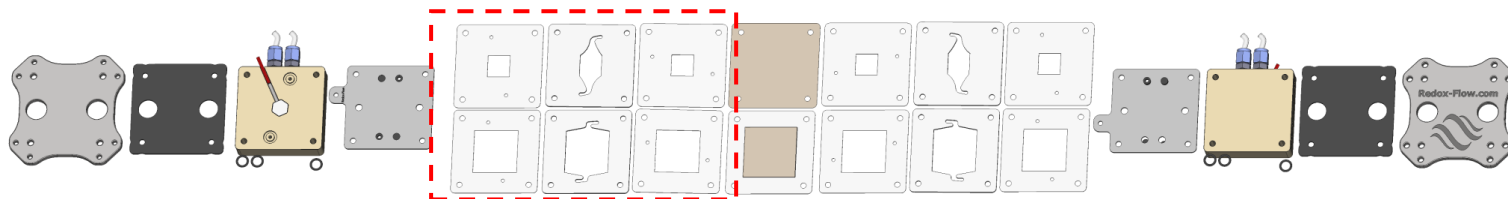

1. Cover/spacer gaskets is placed on current collector

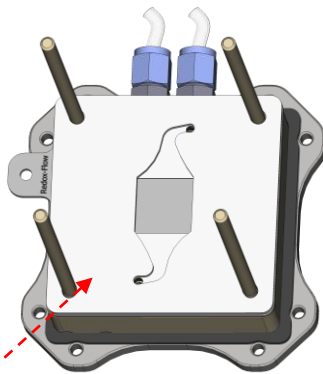

2. Flow field gasket is placed on cover/spacer gasket isolator

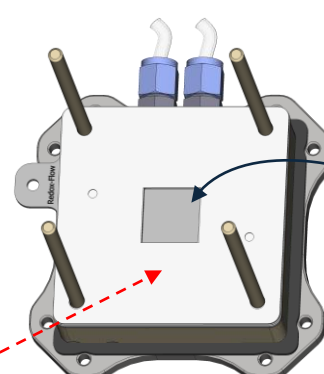


3. Cover/spacer gaskets is mounted



4. Place electrode inside the gaskets

## IMPORTANT NOTES

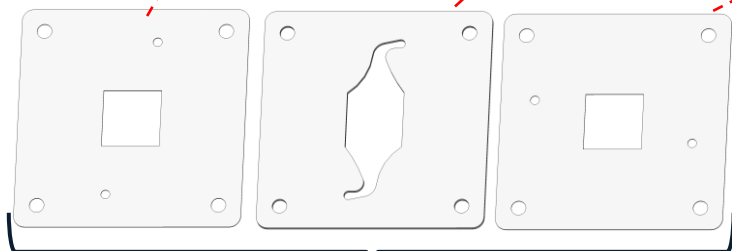


**A.** The final compressed thickness of the electrode is determined by the sum of the thicknesses of all stacked gaskets. Depending on the electrode varying compression is needed to ensure good electrical contact to the current collector

**B.** Several gaskets of both types (flow field and cover) can be stacked on top of each of to fine-tune final compressed electrode thickness

**C.** It is recommended to have the *flow field gasket* as thick as possible and the two *cover/spacer gaskets* as thin as possible - This is to ensure that the hydraulic channels that connects to the reference electrode(s) are as large as possible.


# Assembly - Current collectors with flat surface

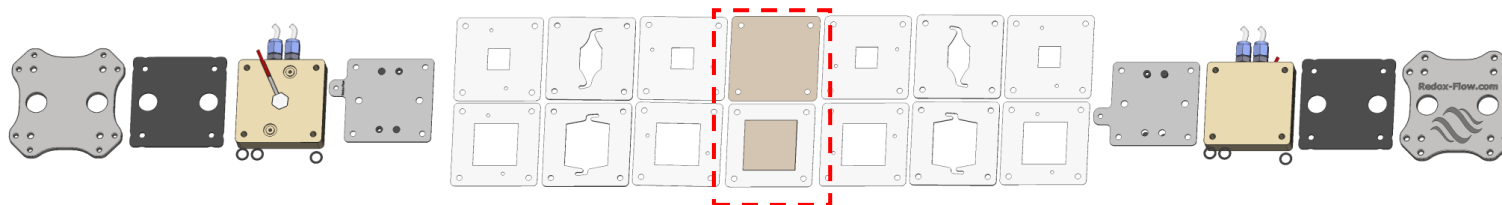

## A. Assembly with porous separators

If the cell is operated with a porous separator use this section. If not go to section B on next page.


For porous separators it is in most cases necessary to include a *porous separator gasket* to prevent leaking out through the side of separator

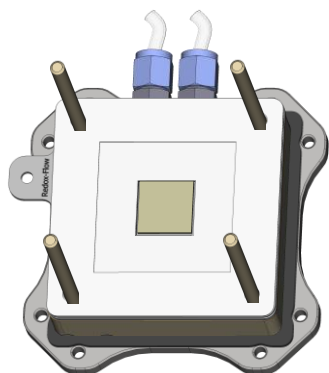

1. The *porous separator gasket* is placed on the previous gaskets NOTE: The open area of the *porous separator gasket* is 60mm x 60mm



2. Cut a 60 mm x 60 mm separator

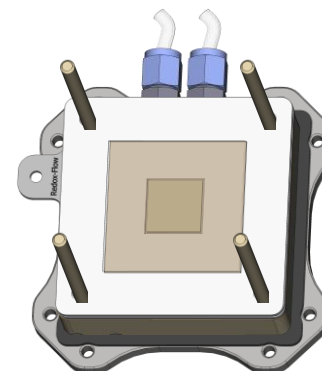


3. Place the separator inside the *porous separator gasket* is

## IMPORTANT NOTES

- A. It is recommended to have a *porous separator gasket* thickness, that has the same thickness or slightly thinner than the thickness of the porous separator (e.g. within 0.0 mm to 0.1 mm)
- B. Several *porous separator gaskets* can be stacked on top of each of to fine-tune final thickness
- C. It is recommended to use either VITON or EPDM (compressible) as the main gasket and fine tune with PTFE gaskets. This will make sealing easier.


# Assembly - Current collectors with flat surface

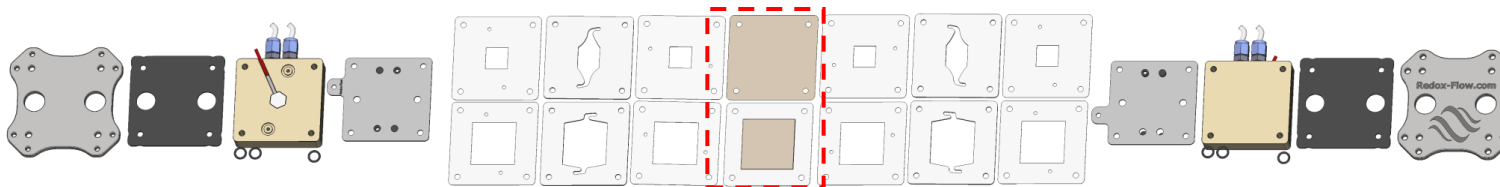

## B. Assembly with dense & thin membranes

If the cell is operated with a dense and thin membrane a *porous separator gasket* is not necessary, and membranes of variable areas can be used.

**1a.** Use a membrane with a minimum dimension of 60 mm x 60 mm





**OR**



**1b.** Use a membrane with the same outer dimensions as the gaskets (approximately 100 mm x 100 mm)

**OR**


**1c.** Use a membrane with any dimension in between 1a and 1b

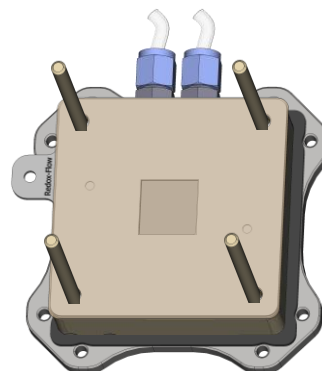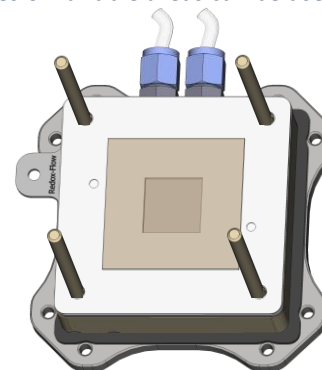


# Assembly - Current collectors with flat surface

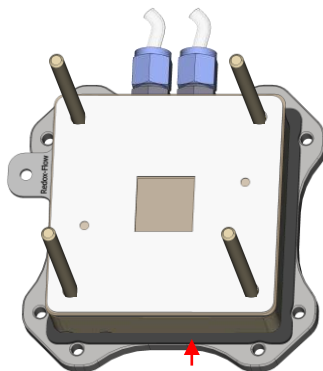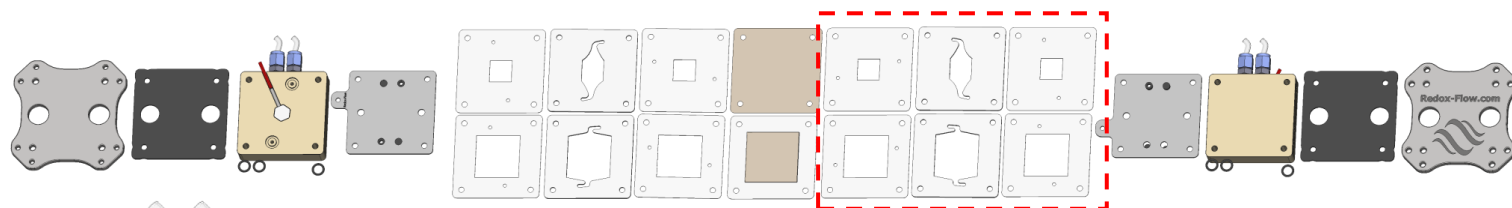

1. Cover/spacer gaskets is placed on membrane

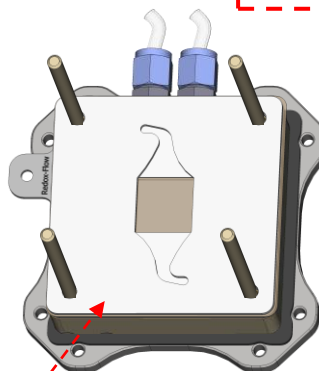


2. Flow field gasket is placed on cover/spacer gasket

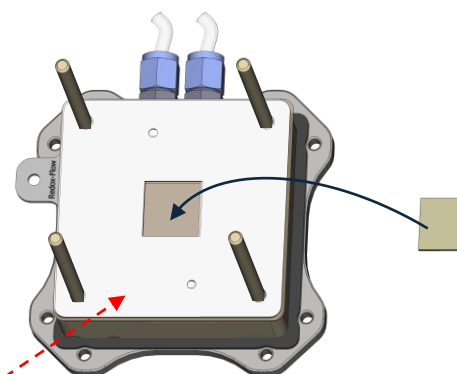

3. Cover/spacer gaskets is placed on Flow field gasket

4. Place electrode inside the gaskets

## IMPORTANT NOTES

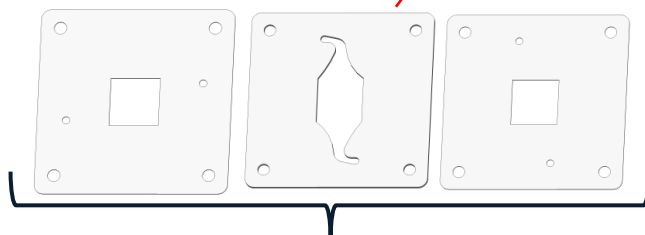



A. The final compressed thickness of the electrode is determined by the sum of the thicknesses of all stacked gaskets. Depending on the electrode varying compression is needed to ensure good electrical contact to the current collector

B. Several gaskets of both types (flow field and cover) can be stacked on top of each of to fine-tune final compressed electrode thickness

C. It is recommended to have the *flow field gasket* as thick as possible and the two *cover/spacer gaskets* as thin as possible - This is to ensure that the hydraulic channels that connects to the reference electrode(s) are as large as possible.




# Assembly - Current collectors with flat surface

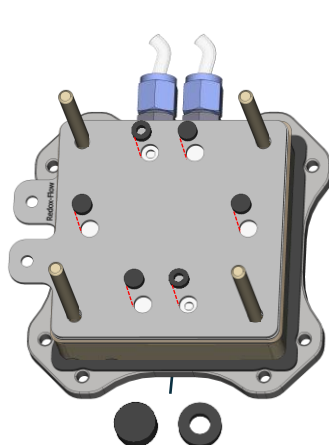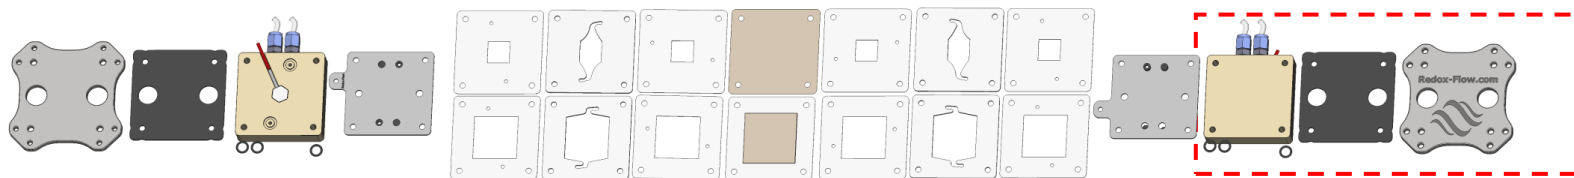


**1.** Current collector is placed on last *Cover/spacer gaskets*  
NOTE: the flow field in the current collector must face downwards

**2.** *Ring gaskets* with and without holes are mounted in current collector. Use  
NOTE: Use *Ring gaskets* with holes where there is a port and *Ring gaskets* without holes in the holes without ports.

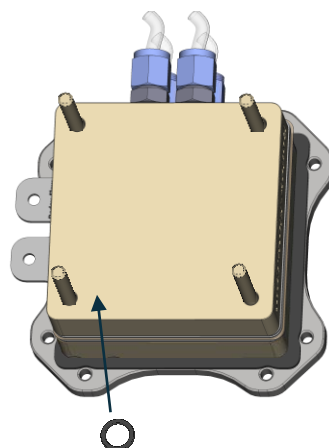


**3.** All three O-rings are mounted in the PEEK flow body (opposite side)  
NOTE: If a thermometer is also used on this side, the thermometer holder should also be mounted.

**4.** PEEK flow body is placed on current collector

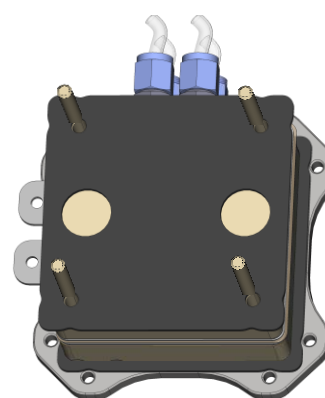

**5.** Isolator is placed on PEEK flow body


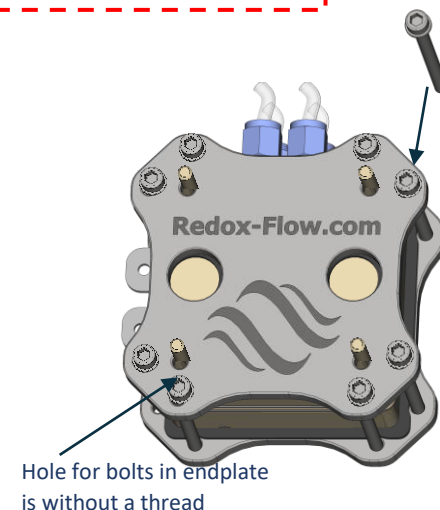


**6.** Unthreaded endplate is placed with logo downwards

**7.** All eight bolts are placed in the outmost holes in the endplate  
NOTE: Use bolts with correct length  
NOTE: Keep alignment bars in the cell – they are taken out during the tightening of the cell


CELL IS NOW ASSEMBLED AND READY FOR TIGHTENING

# Assembly - Current collectors with flow field

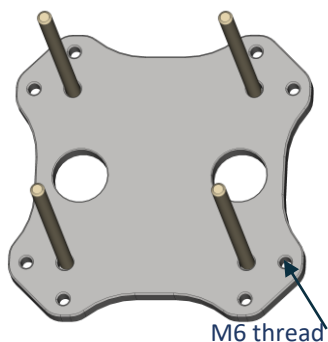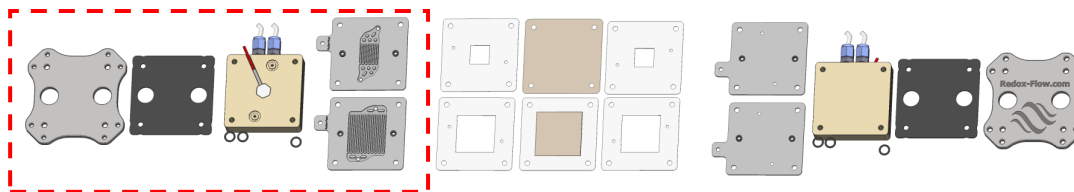


1. Threaded endplate is placed with logo downwards

2. All four alignment bars are placed in the holes in the endplate

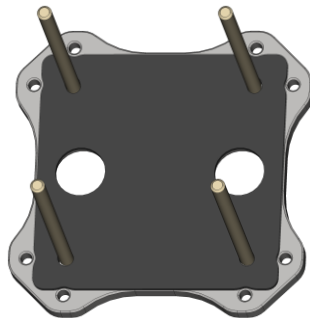


3. Isolator is placed on endplate

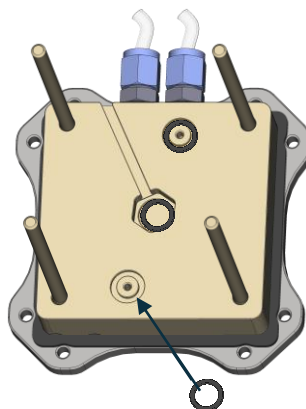


4. PEEK flow body is placed on isolator

5. All three O-rings are mounted in the PEEK flow body

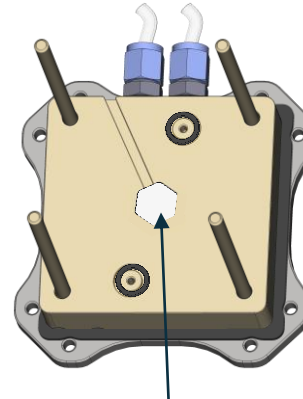


6. Alu thermometer holder is placed in the center hole

NOTE: The holder comes with three holes with different diameter.  
-Choose the hole that fits your thermometer best  
-Make sure the hole points toward the groove in the PEEK plate  
-To ensure good thermal contact a little grease can be applied in the hole.


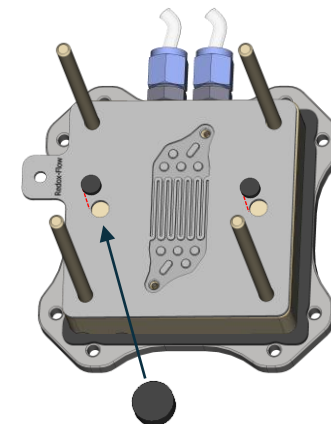


7. Current collector is placed on PEEK flow body

8. Ring gaskets without holes are mounted in current collector

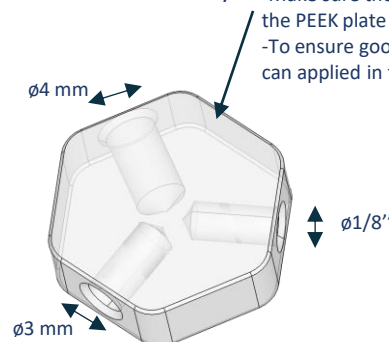


# Assembly - Current collectors with flow field

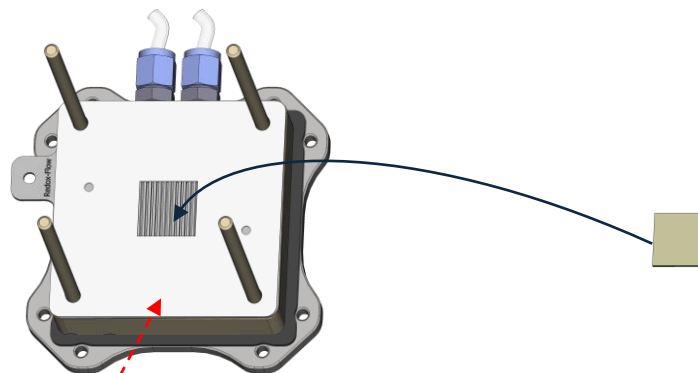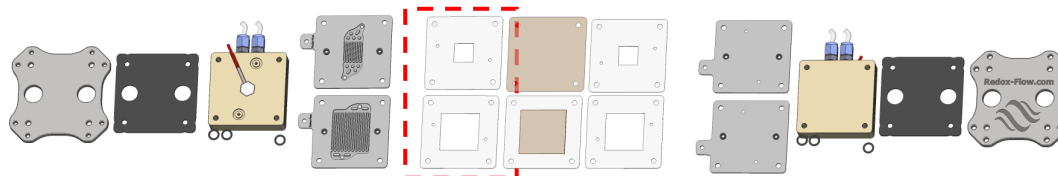

1. Cover/spacer gaskets is placed on current collector

2. Place electrode inside the gaskets


## IMPORTANT NOTES



**A.** The final compressed thickness of the electrode is determined by the sum of the thicknesses of all stacked gaskets. Depending on the electrode varying compression is needed to ensure good electrical contact to the current collector

**B.** Several gaskets can be stacked on top of each of to fine-tune final compressed electrode thickness


# Assembly – current collectors with flow field

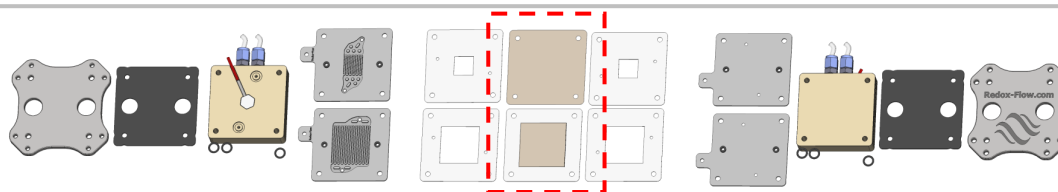

## A. Assembly with porous separators

If the cell is operated with a porous separator use this section. If not go to section B on next page.


For porous separators it is in most cases necessary to include a *porous separator gasket* to prevent leaking out through the side of separator

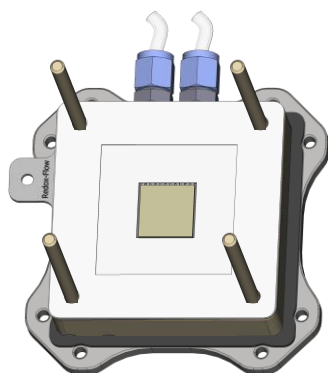

1. The *porous separator gasket* is placed on the previous gaskets NOTE: The open area of the *porous separator gasket* is 60mm x 60mm



2. Cut a 60 mm x 60 mm separator

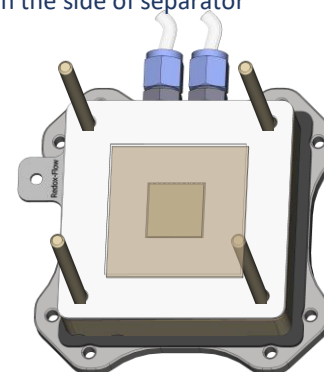


3. Place the separator inside the *porous separator gasket*

## IMPORTANT NOTES

- A. It is recommended to have a *porous separator gasket* thickness, that has the same thickness or slightly thinner than the thickness of the porous separator (e.g. within 0.0 mm to 0.1 mm)
- B. Several *porous separator gaskets* can be stacked on top of each of to fine-tune final thickness
- C. It is recommended to use either VITON or EPDM (compressible) as the main gasket and fine tune with PTFE gaskets. This will make sealing easier.


# Assembly – current collectors with flow field

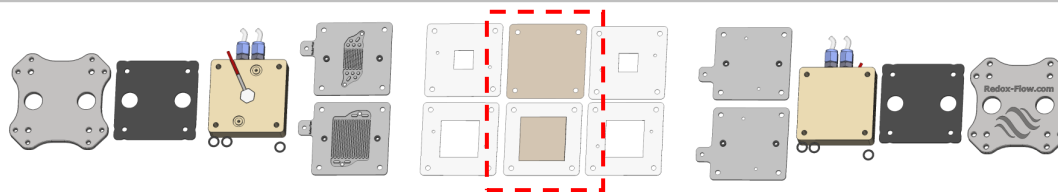

## B. Assembly with dense & thin membranes


If the cell is operated with a dense and thin membrane a *porous separator gasket* is not necessary, and membranes of variable areas can be used.

**1a.** Use a membrane with a minimum dimension of 60 mm x 60 mm





**OR**

**1b.** Use a membrane with the same outer dimensions as the gaskets (approximately 100 mm x 100 mm)





**OR**

**1c.** Use a membrane with any dimension in between 1a and 1b

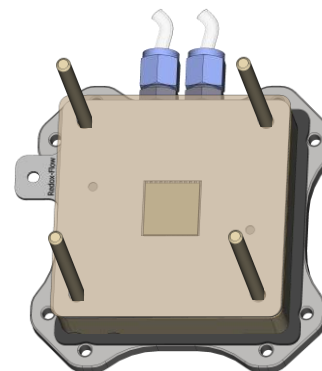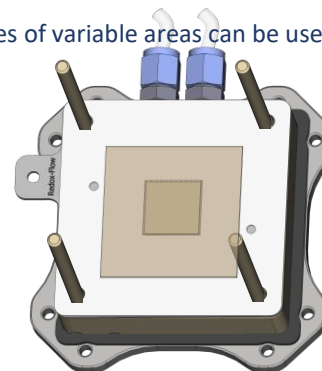


# Assembly - Current collectors with flow field

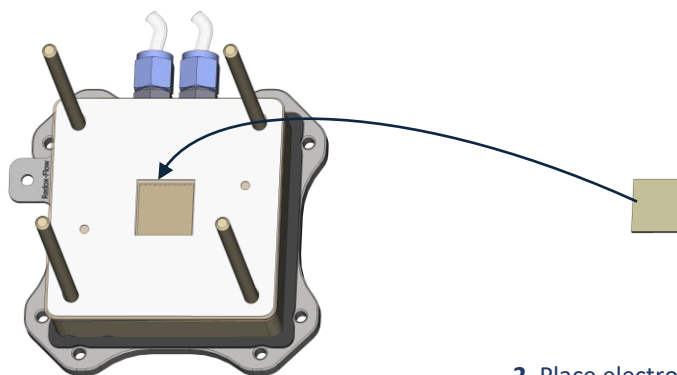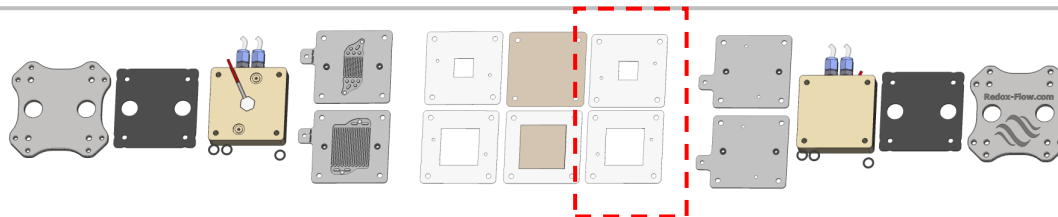

1. Cover/spacer gaskets is placed on membrane.

2. Place electrode inside the gaskets



## IMPORTANT NOTES



**A.** The final compressed thickness of the electrode is determined by the sum of the thicknesses of all stacked gaskets. Depending on the electrode varying compression is needed to ensure good electrical contact to the current collector


**B.** Several gaskets can be stacked on top of each of to fine-tune final compressed electrode thickness

# Assembly - Current collectors with flow field

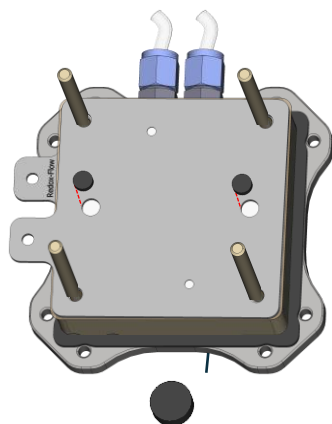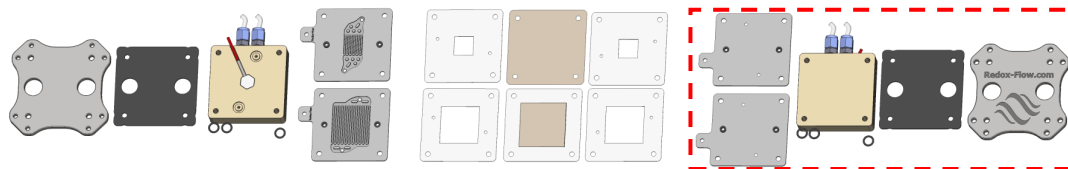


**1.** Current collector is placed on last *Cover/spacer gaskets*  
NOTE: the flow field in the current collector must face downwards

**2.** Ring gaskets without holes are mounted in current collector

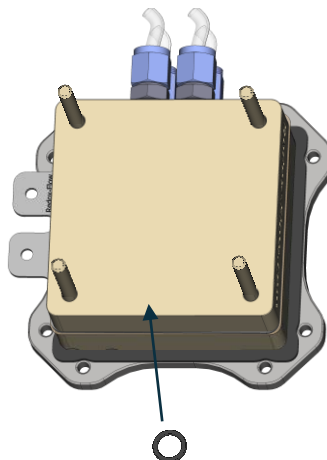


**3.** All three O-rings are mounted in the PEEK flow body (opposite side)  
NOTE: If a thermometer is also used on this side, the thermometer holder should also be mounted.

**4.** PEEK flow body is placed on current collector

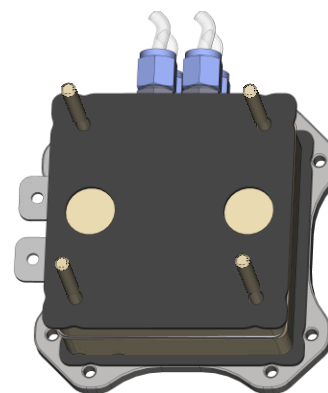

**5.** Isolator is placed on PEEK flow body

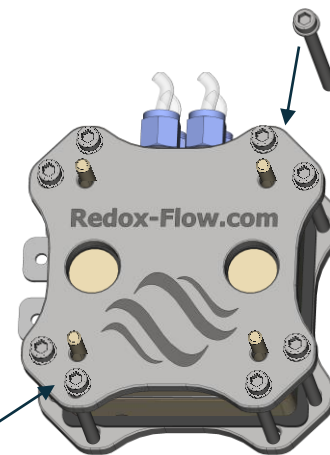

Hole for bolts in endplate is without a thread

**6.** Unthreaded endplate is placed with logo upwards

**7.** All eight bolts are placed in the outmost holes in the endplate  
NOTE: Use bolts with correct length  
NOTE: Keep alignment bars in the cell – they are taken out during the tightening of the cell

CELL IS NOW ASSEMBLED AND READY FOR TIGHTENING

# Assembly – Final assembly




## STEP 1

- Hex bolts are cross tightened up to 6 Nm.
- Alignment bars are removed before cell is completely tightened - if left in the cell, there is a (small) risk of leaks inside channels for the alignment bars

## IMPORTANT NOTES

- Measurement with caliber is paramount for a tight sealing – It is not a high torque that seals the cell, it is a correct alignment of the flow bodies

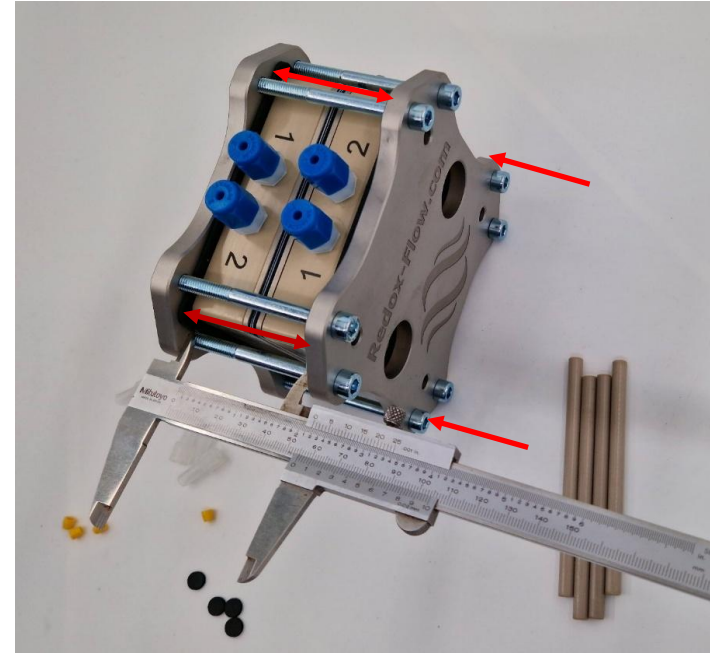


## STEP 2

- Quality of the cross tightened is checked by measuring the distance between the endplates at all four corners with a caliber
- The distance should not vary more than 0.1-0.2mm
- NOTE: Step 1 and 2 can be performed iteratively.



# Application notes – Electrical connections

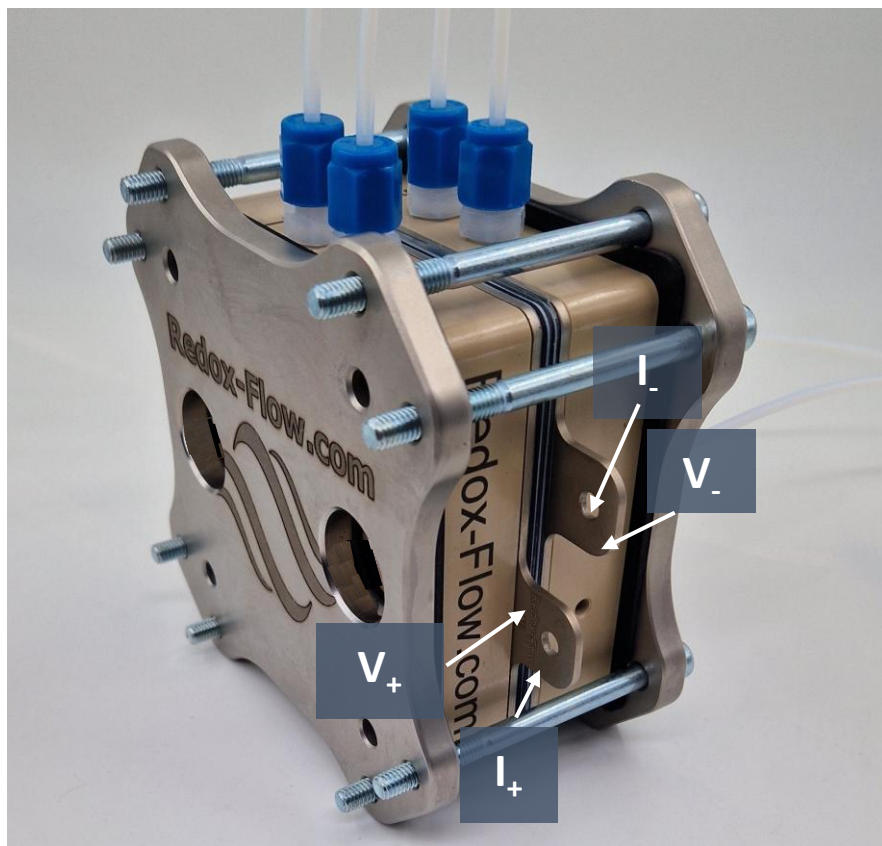

Voltage measurement and current connections

**IMPORTANT** - It is paramount for safety and reproducible data that the wires for


- Electrical current ( $I_+$  and  $I_-$ ) are well connected on the current collectors e.g. with cable lugs, bolts or other recognized solutions for making proper electrical connections

**NOTE:** Poorly connected current wires will lead to significant contact resistance between the wire and current collectors. For high current operation (e.g.  $> 1$  A) the contact resistance (even small ones) can lead to significant heating in the contact points.

- Voltage measurements ( $V_+$  and  $V_-$ ) are mounted on the current collectors to ensure a proper 4-wire configuration

**NOTE:** As the wires for voltage measurement does not carry any electrical current, there are no strict requirements for the quality of the connection and can e.g. be connected with crocodiles or similar

# Application notes – Temperature sensors

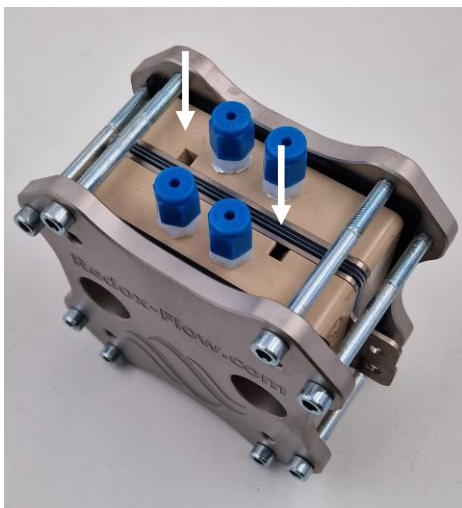


Holes for thermometers


## Temperature sensor

- In each of the PEEK flow bodies there are holes with direct access to the aluminum thermometer holder. The distance from the PEEK surface to the bottom of the thermometer holder is approximately 55 mm
- The aluminum holder is pressed up against the metal current collector. This ensures very good thermal contact whereby
  - The temperature can be measured fast (very short time delay on temperature changes)
  - The temperature can be measured very precise
- To increase the thermal contact a little grease can be applied to the head of the thermometer or inside the hole of the thermometer holder


**VERY IMPORTANT:** The thermometer holder is in direct metallic contact with the bipolar plate and will for this reason have the same applied electrical potential as the bipolar plate. **Here is it extremely important that the electrical circuit of the thermometer is electrically isolated from the metal parts.** This is the case for most thermometers with housings (even metallic ones) but can be tested by measuring the electrical resistance with a multimeter between thermometer housing and thermometer measurement wires. However, this is not the case for bare/unprotected thermometer, these can be isolated with tape, shrinking tube or similar.

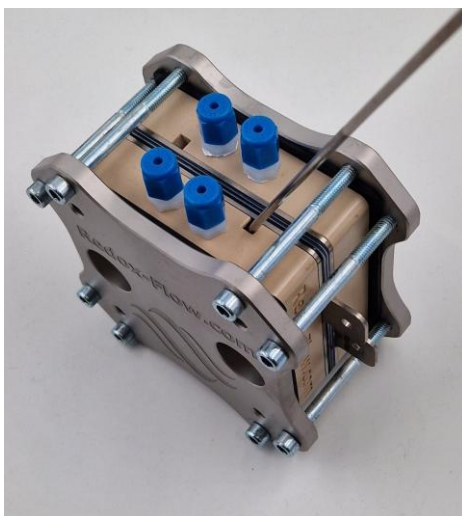


Mounting with rigid thermometer

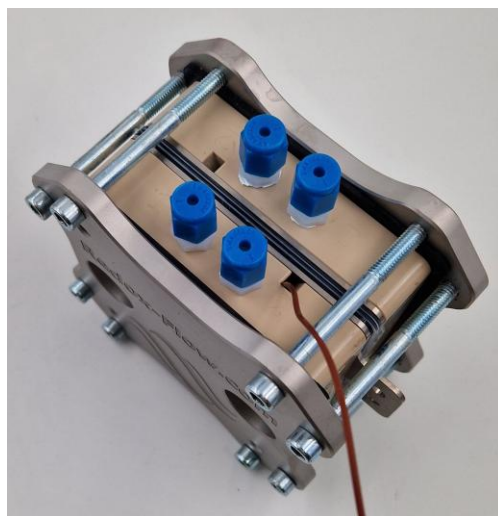

Mounting with wire thermometer

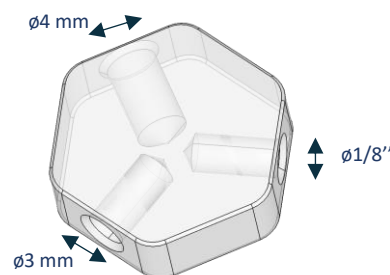


Thermometer holder

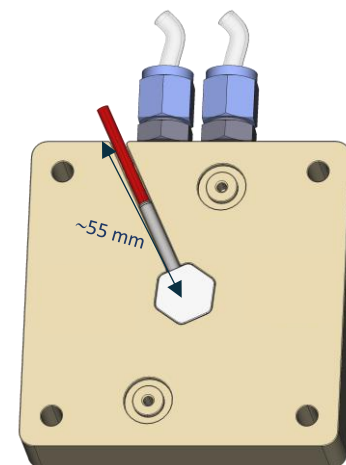

Thermometer, holder & PEEK block (metal current collector is mounted on top)

## Application notes – Hydraulic connections

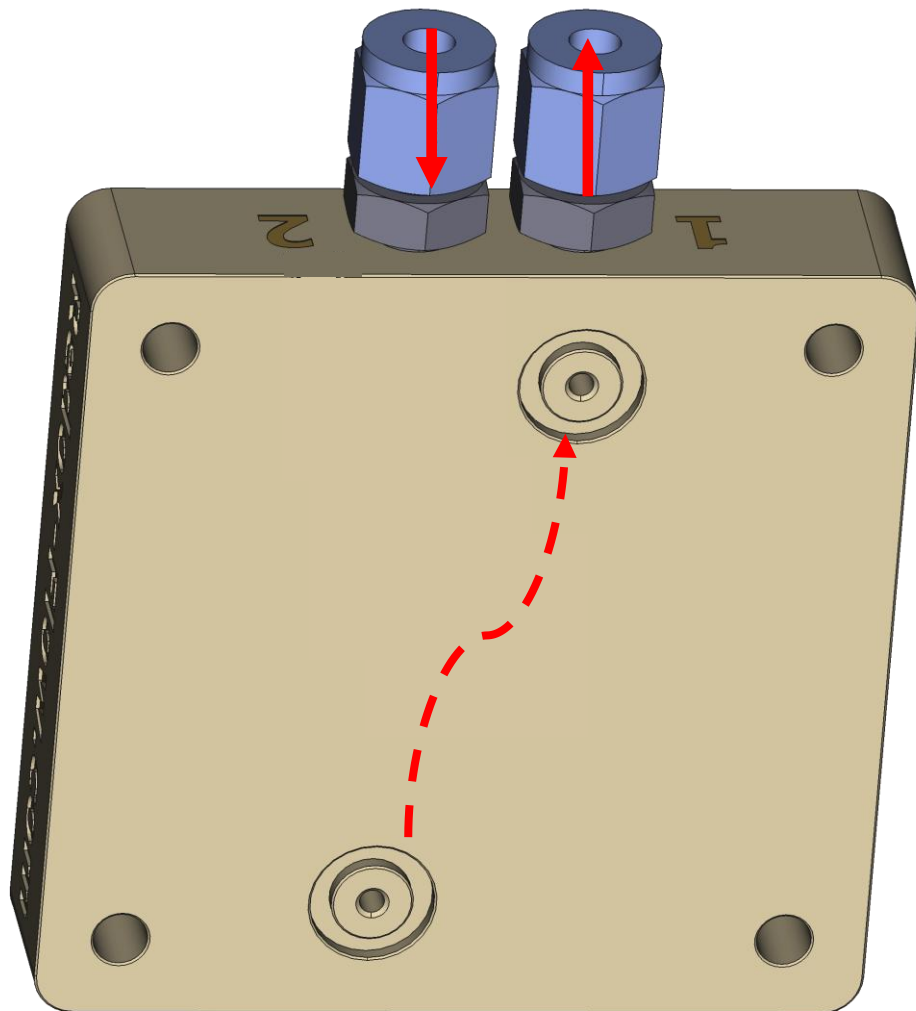

For normal operation it is recommended to use **port 1** as outlet of for the liquid and **port 2** as the inlet for the liquid

NOTE: With this configuration the liquid enters at the bottom and exits at the top. This makes removal of bubbles easier.